

Scattering Meter

ECO-BB

User's Guide

This user's guide is an evolving document. If you find sections that are unclear or missing information, please let us know. Please check our website periodically for updates.

WET Labs, Inc. PO Box 518 Philomath, OR 97370 (541) 929-5650 wetlabs@wetlabs.com www.wetlabs.com



Attention!

Return Policy for Instruments with Anti-fouling Treatment

WET Labs cannot accept instruments for servicing or repair that are treated with anti-fouling compound(s). This includes but is not limited to tri-butyl tin (TBT), marine anti-fouling paint, ablative coatings, etc.

Please ensure any anti-fouling treatment has been removed prior to returning instruments to WET Labs for service or repair.



ECO Sensor Warranty

This unit is guaranteed against defects in materials and workmanship for a period of one year after the original date of purchase. WET Labs will supply all replacement parts and labor and pay for return via 3rd day air shipping in honoring this warranty. This warranty is considered void if the factory determines that the unit was subjected to abuse or neglect beyond the normal wear and tear of field deployment, or in the event the pressure cans have been opened by the customer (this does not apply to pressure cans on battery-supplied units). The customer should call for a Return Manufacturer's Authorization (RMA) before returning the instrument to the factory and is responsible for shipping costs to WET Labs. WET Labs is not responsible for shipping damage done during the return shipment. WET Labs assumes no liability for equipment damage, personal injury or loss of data resulting from use of this instrument, except for that stated in this warranty.



Table of Contents

1. Specificat	tions	1
1.1 Con	nectors	2
1.2 Test	: Cable	3
1.3 Deliv	vered Items	3
1.4 Bio-\	Wiper™	4
1.5 Batte	eries	4
2. Theory of	Operation	5
3. Instrumen	nt Operation	6
3.1 Initia	al Checkout	6
3.2 Ope	rating the Sensor for Data Output	6
3.3 Depl	loyment	7
3.4 Upke	eep and Maintenance	7
3.5 <i>Bio-</i> 1	wiper™ Operation	8
4. BBB/BBS	B: Using Internal Batteries	11
	noving End Flange and Batteries	
	lacing End Flange and Batteries	
• • • • • • • • • • • • • • • • • • •	cking Vent Plug	
	lysis	
	a Corrections	
5.2 Deriv	ved Parameters	15
6. Testing ar	nd Calibration	16
6.1 Test	ting	16
6.2 Calib	bration	17
Definitions of	of Terms	17
7. Terminal	Communications	18
	face Specifications	
	nmand List	
8 Device Fil	les	10
	Header	
	ımn Count Specification	
	umn Description	
	nple Device File	
	ple Output File	
A	Mayorting Decelet December	0.4
Appendix A:	Mounting Bracket Drawing	21



1. Specifications

Model	BB(RT)	BB(RT)D	ВВ	BBB	BBS	BBSB
Mechanical						
Diameter	2.48 in (6.3 cm)	2.48 in (6.3 cm)	2.48 in (6.3 cm)	2.48 in (6.3 cm)	2.48 in (6.3 cm)	2.48 in (6.3 cm)
Length	5.0 in (12.7 cm)	7.0 in (17.8 cm)	5.0 in (12.7 cm)	10.0 in (25.4 cm)	5.25 in (13.3 cm)	10.25 in (26.0 cm)
Weight in air	0.9 lbs (0.4 kg)	0.9 lbs (0.4 kg)	0.9 lbs (0.4 kg)	2.1 lbs (0.96 kg)	1.1 lbs (0.5 kg)	2.1 lbs (0.96 kg)
Weight in water	0.05 lbs (0.02 kg)	1.66 lbs (0.75 kg)	0.05 lbs (0.02 kg)	0.3 lbs (0.14 kg)	0.19 lbs (0.08 kg)	0.3 lbs (0.14 kg)
Material	ABS	ABS	Titanium	ABS	ABS	ABS
Environmental						
Temperature range	0–30 deg C	0–30 deg C	0–30 deg C	0–30 deg C	0–30 deg C	0–30 deg C
Depth rating	600 m	600 m	6000 m	600 m	300 m	300 m
Temperature/pressure sensor (optional)	Y	Y	Y	Υ	Υ	Υ
Electrical						
Digital output resolution	12 bits	12 bits	12 bits	12 bits	12 bits	12 bits
Analog output signal	0–5 V	0–5 V	0–5 V	0–5 V	0–5 V	0–5 V
Internal data logging	N	N	Υ	Υ	Y	Y
Internal batteries	N	N	N	Y	N	Y
Connector	MCBH6M	MCBH6M	MCBH6M	MCBH6M	MCBH6M	MCBH6M
Input	7-15 VDC	7-15 VDC	7-15 VDC	7-15 VDC	7-15 VDC	7–15 VDC
Current, typical	80 mA	80 mA	80 mA	80 mA	80 mA	80 mA
Current, sleep		85 µA		85 µA	85 µA	85 µA
Data memory		1 MB (65,000 samples)		1 MB (65,000 samples)	1 MB (65,000 samples)	1 MB (65,000 samples)
Sample rate	to 10 Hz	to 10Hz	to 10 Hz	To10 Hz	to 10 Hz	to 10 Hz
RS-232 output	19200 baud	19200 baud	19200 baud	19200 baud	19200 baud	19200 baud
Anti-fouling bio- wiper™	N	N	N	N	Y	Y
Bio-wiper™ cycle					110 mA	110 mA
Optical						
Wavelength (nm)	470, 530, or 660 (880 optional)	470, 530, or 660 (880 optional)	470, 530, or 660 (880 optional)	470, 530, or 660 (880 optional)	470, 530, or 660 (880 optional)	470, 530, or 660 (880 optional)
Resolution, blue	4.1 x 10 ⁻⁵ m ⁻¹ sr ⁻¹	4.1 x 10 ⁻⁵ m ⁻¹ sr ⁻¹	4.1 x 10 ⁻⁵ m ⁻¹ sr ⁻¹	4.1 x 10 ⁻⁵ m ⁻¹ sr ⁻¹	4.1 x 10 ⁻⁵ m ⁻¹ sr ⁻¹	4.1 x 10 ⁻⁵ m ⁻¹ sr ⁻¹
Resolution, green	5.6 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	5.6 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	5.6 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	5.6 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	5.6 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	5.6 x 10 ⁻⁶ m ⁻¹ sr ⁻¹
Resolution, red	2.1 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	2.1 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	2.1 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	2.1 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	2.1 x 10 ⁻⁶ m ⁻¹ sr ⁻¹	2.1 x 10 ⁻⁶ m ⁻¹ sr ⁻¹
Sensitivity, (min)	0.005 m ⁻¹ @ 1 Hz	0.005 m ⁻¹ @ 1 Hz	0.005 m ⁻¹ @ 1 Hz	0.005 m ⁻¹ @ 1 Hz	0.005 m ⁻¹ @ 1 Hz	0.005 m ⁻¹ @ 1 Hz
Linearity	99% R ²	99% R ²	99% R ²	99% R ²	99% R ²	99% R ²



BB(RT)— Provides analog or RS-232 serial output with 4,000-count range. This unit provides continuous operation when power is supplied.

BB—Provides the capabilities of the BB(RT) with periodic sampling

BBD—Provides the capabilities of the BB(RT) with 6,000-meter depth rating.

BBB—Provides the capabilities of the BB with internal batteries for autonomous operation.

BBS—Provides the capabilities of the BB with an integrated anti-fouling *bio-wiper*™.

BBSB—Provides the capabilities of the BBS with internal batteries for autonomous operation.

1.1 Connectors

ECO-BB instruments use a six-pin bulkhead connector as shown in Figure 1. Table 1 summarizes pin functions for the bulkhead connectors.

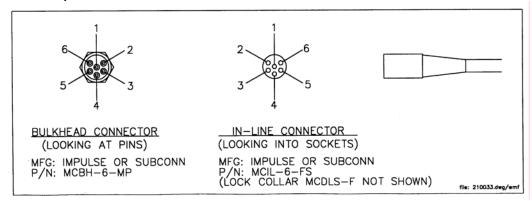


Figure 1. *ECO*-BB connector schematic

Table 1. Pinout summary for *ECO* BB connectors

Pin (or Socket)	Function	Function
	BB(RT) and BB(RT) (deep)	BB, BBB, BBS, BBSB
1	Ground	Ground
2	Reserved	RS-232 (RX)
3	Reserved	Reserved
4	V in	V in
5	Reserved	RS-232 (TX)
6	Analog out	Reserved

WARNING

If you are going to build or use a non-WET Labs-built cable, do not use the wire from pin 3 or the *ECO* meter will be damaged.

Input power of 7.5–15 VDC is applied to pin 4. The power supply current returns through the common ground pin. The input power signal has a bi-directional filter. This prevents external power supply noise from entering into *ECO*-BB, and also prevents internally generated noise from coupling out on to the external power supply wire. Note that the power



supply and the analog output share a common ground. The BBD (deep) mechanical case is floating; it is not connected to the ground.

1.1.1 ECO BBB and BBSB Connectors

ECO BBB and BBSB (units with internal batteries) have an second bulkhead connector that comes with a jumper plug to supply power to the unit. The pin functions for this connector are shown in Figure 2. Table 2 summarizes pin functions for the 3-socket bulkhead connector.

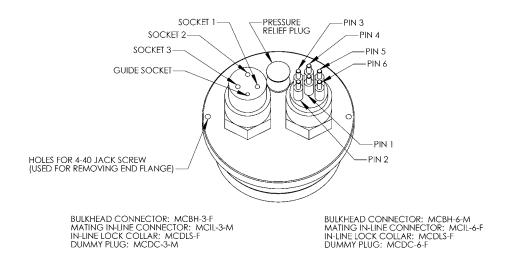


Figure 2. ECO BBB and BBSB connector schematic

Table 2. Pinout summary for *ECO* 3-socket connector

Pin (or Socket)	Function
1	V in
2	N/C
3	Battery out

1.2 Test Cable

A test cable is supplied with each unit. This cable includes four legs:

- 1. A power interface module provides power to the instrument from the connected 9 V battery.
- 2. An auxiliary analog out connector.
- 3. A DB-9 serial interface connector.
- 4. A six-socket in-line connector plugs into the sensor to provide power and obtain signal.

1.3 Delivered Items

The standard ECO delivery consists of the following:

• the instrument itself



- test cable
- protective cover for optics
- dummy plug with lock collar
- this user's guide
- ECOView user's guide
- ECOView host program and device file (on CD)
- instrument-specific calibration sheet
- BB(RT), BB, BBS: stainless steel mounting bracket and hardware (See Appendix A for details)
- One 0.050-in. hex key for bio-wiperTM removal (units with bio-wiperTM only)
- spare parts kit (battery units only):
 - □ Two end flange O-rings (size 224)
 - □ Two vent plug O-rings (size 010)
 - □ Two jacking screws for connector flange removal
 - □ One 3/32-in. hex key for jacking screws
 - □ Power plug for autonomous operation
 - □ Three pre-cut segments (7 inches) of 0.036-inch diameter monofilament for end flange
 - □ Three pre-cut segments (0.25 inches) of 0.094-inch diameter white nylon bar stock for replacing the white plastic dowel pin.

1.4 Bio-Wiper™

The BBS and BBSB include an integrated anti-fouling *bio-wiper*TM for use in extended deployments. This *bio-wiper*TM can be manually controlled by a host controller package, or can perform autonomously as part of a pre-programmed sampling sequence upon instrument power-up. The rate of closure and opening is dependent upon both temperature and depth.

1.5 Batteries

The BBB and BBSB incorporate six 9-volt batteries as their internal power source. They can either use standard alkaline cells for a total capacity of approximately 1000 mA-hrs, or for longer deployments can use LiMnO₂ cells to achieve more than 2000 mA-hrs of operational capacity. Actual total usage time of the internal batteries is a function of several parameters. These include nominal water temperature, sequence timing, sample periods, and total deployment duration.

WARNING!

Pin 6 is always "hot." Be sure to keep the dummy plug on the BBB and BBSB when not in use.

For even greater deployment capability contact WET Labs for information on external battery packs.



2. Theory of Operation

The *Environmental Characterization Optics*, or *ECO* miniature scattering meter allows the user to measure scattering at 117 degrees. This angle was determined as a minimum convergence point for variations in the volume scattering function induced by suspended materials and water itself. Therefore, the signal measured by this meter is less determined by the type and size of materials in the water and more directly correlated to the concentration of the materials.

The *ECO* uses one LED (modulated at 1 kHz) source light. The source light enters the water volume and scattered material is detected by a detector positioned where the acceptance angle forms a 117-degree intersection with the source beam. Figure 3 shows the optical configuration for the *ECO*-BB.

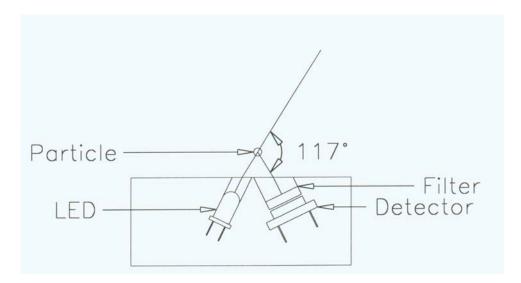


Figure 3. Optical configuration of ECO scattering meter



3. Instrument Operation

Please note that certain aspects of instrument operation are configuration-dependent. These are noted where applicable within the manual.

3.1 Initial Checkout

Supplied from the factory, *ECO*s are configured to begin continuously sampling upon power-on. Electrical checkout of *ECO* is straightforward.

Connect the 6-socket connector on the test cable to the instrument to provide power to the LEDs and electronics (see Section 1 for a diagram of the pinouts of *ECO*-BB). Connect the battery leads on the test cable to the 9V battery supplied with the meter. Light should emanate from the meter.

3.1.1 Analog Option

Connect a digital multimeter (DMM) to the auxiliary leg of the test cable: the center of the RCA connector provides analog out signal and the outside provides ground. With the sensor face clean and dry the instrument should read approximately 0.050–0.095 VDC. The analog signal will saturate at 5 volts.

3.2 Operating the Sensor for Data Output

Note

ECO scattering meters are sensitive to AC light. Before making measurement, turn AC lighting off.

1. Connect the 6-socket connector to the instrument to provide power to the LEDs and electronics. Connect the DB-9 connector to a computer with the ECOView host program installed on it.

WARNING!

Always use a regulated power supply to provide power to ECO sensors if not using the 9V battery provided with the test cable: power spikes may damage the meter.

- 2. Start ECOView. Select the appropriate COM Port and Device File. Supply power to the meter, then click on the Start Data button. Output will appear in the Raw Data window. Place the flat of your hand in front of the sensor face and note that the signal will increase toward saturation (maximum value on calibration sheet) as your hand gets closer. When applying power to sensors with a *bio-wiper*TM, it will open and, depending on the settings, operate until you select Stop Data in ECOView (or input !!!! in a terminal program) The *bio-wiper*TM will close and the instrument will await the next command.
- 3. If the sensor completes the requested samples (this is common for meters set up in moored applications), it will go into sleep mode, and the meter will not light when power



is cycled. To "wake" the meter, click Stop Data five times at the rate of two times per second immediately upon applying power. This interrupts the sensor, returning it to a "ready" state, awaiting commands.

- 4. Check the settings for the ECO and change if necessary. ECOView factory settings for continuous operation:
 - Set Number of Samples = 0
 - Set Number of Cycles = 0.
- 5. If the meter does not light after performing step 3, check the battery. Replace if necessary, perform steps 2 and 3 to verify communication. If it still does not light, contact WET Labs.

Refer to the ECOView User's Guide for details about using the software.

3.3 Deployment

The *ECO* scattering meter requires no pump to assure successful operation. Once power is supplied, the unit is ready for submersion and subsequent measurements. Some consideration should be given to the package orientation. Do not face the sensor directly into the sun or other bright lights. For best output signal integrity, locate the instrument away from significant EMI sources.

Caution

The BB should be mounted so that the LED source will not "see" any part of a cage or deployment hardware. This will affect the sensor's output.

Other than these basic considerations, one only needs to make sure that the unit is securely mounted to whatever lowering frame is used and that the mounting brackets are not damaging the unit casing. The instrument can be used in a moored or profiling mode.

3.4 Upkeep and Maintenance

The *ECO*-BBs are compact devices and their maintenance can be easily overlooked. However, it is a precision instrument and does require a minimum of routine upkeep. After each cast or exposure of the instrument to natural water, flush the instrument with clean fresh water, paying careful attention to the sensor face. Use soapy water to cut any grease or oil accumulation. Gently wipe clean with a soft cloth. The sensor face is composed of ABS plastic and optical epoxy and can easily be damaged or scratched.

WARNING

Do not use acetone or other solvents to clean the sensor.

At the end of an experiment, the instrument should be rinsed thoroughly, air-dried and stored in a cool, dry place.



3.5 *Bio-wiper™* Operation

The *ECO*-BBS and -BBSB are provided with an anti-fouling *bio-wiper*TM. The *bio-wiper*TM extends the possible deployment duration by retarding biological growth on the instrument's optical surface. The *bio-wiper*TM covers the optical surface: 1) while the instrument is in "sleep" mode; 2) when it has completed the number of samples requested; and 3) when the user selects **Stop Data** in ECOView or types "!!!!!" in a terminal program. When the meter wakes up, the optical surface is exposed by the *bio-wiper's*TM counter-clockwise rotation.



If power is shut off in mid cycle, the *bio-wiper*TM will reinitialize to the beginning of the user-selected settings when power is applied again.

3.5.1 *Bio-wiper*TM Cleaning and Maintenance

When not in active sample mode, the bio-wiperTM can be removed by using the factory-supplied 0.050 hex key to loosen the set screw that attaches the shutter to the instrument. Take care to ensure no unnecessary torque is placed on the shaft.

To clean, wash in soapy water, rinse and dry thoroughly. Note the condition of the copper on the instrument side of the shutter. It is normal for the copper *bio-wiper*TM to corrode and turn green, especially after the instrument has been removed from the water. This corrosion will slightly reduce the shutter's antifouling ability the next time it is deployed. For maximum antifouling capability:

- 1. Remove *bio-wiper*TM
- 2. Buff with a pad of green Scotch Brite® (or similar) until shiny
- 3. Re-install *bio-wiper*TM

When re-installing the *bio-wiper*TM on the instrument, the wiper blade must be properly flexed. To achieve the proper flex of the wiper, set the gap between the copper *bio-wiper*TM and the instrument face to 0.03 in. (0.8 mm). An improperly set gap will either fail to clean the face, or cause the motor to draw excessive current (Figure 4).

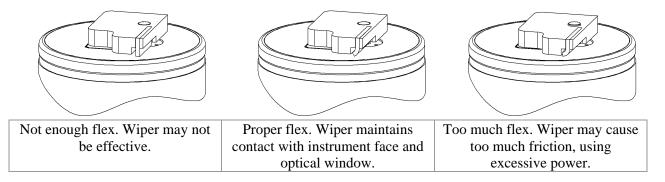


Figure 4. Adjusting bio-wiperTM for proper flex

To set this gap:

- 1. Fold a piece of paper in half, then in half again, then fold a third time, creasing the edges. It's now 8 sheets thick and about 0.03 in. thick.
- 2. Make sure the *bio-wiper*TM is in the closed position. You may have to run the instrument.
- 3. If it is not already loosened, loosen the set screw holding the *bio-wiper*TM and put the paper gage between the instrument face and the bio-wiper.



- 4. Push down on the bio-wiperTM and rotate it counter-clockwise so that the shutter is in the closed position.
- 5. Without letting the wiper spring up, tighten the set screw.
- 6. Run the instrument to verify operation



4. BBB/BBSB: Using Internal Batteries

ECO sensors powered with internal batteries can either run directly from the internal batteries or can operate from power supplied by an external DC power supply (7–15 volts). Internal-to-external source conversion is facilitated by a jumper plug that plugs into the unit's bulkhead connector. When inserted, the plug forms a connection from the battery to the electronics power supply. By removing the plug, the instrument can be powered and communicate via a test or deployment cable. Setup conditions, instrument checkout, real-time operation, and data downloading are thus all achieved identically to the methods prescribed for the BB unit.

4.1 Removing End Flange and Batteries

WARNING!

Changing the batteries will require opening the pressure housing of the ECO sensor. Only people qualified to service underwater oceanographic instrumentation should perform this procedure. If this procedure is performed improperly, it could result in catastrophic instrument failure due to flooding or in personal injury or death due to abnormal internal pressure as a result of flooding.

WET Labs Inc. disclaims all product liability from the use or servicing of this equipment. WET Labs Inc. has no way of controlling the use of this equipment or of choosing qualified personnel to operate it, and therefore cannot take steps to comply with laws pertaining to product liability, including laws that impose a duty to warn the user of any dangers involved with the operation and maintenance of this equipment. Therefore, acceptance of this equipment by the customer shall be conclusively deemed to include a covenant by the customer to defend and hold WET Labs Inc. harmless from all product liability claims arising from the use and servicing of this equipment. Flooded instruments will be covered by WET Labs Inc. warranties at the discretion of WET Labs, Inc.

- 1. Make sure the instrument is thoroughly dry.
- 2. Remove the dummy plugs.
- 3. With connector end flange pointed downwards away from face, release seal from vent plug.
- 4. Remove moisture from vent plug area.
- 5. Using needle nose pliers, remove filament from end flange.
- 6. Lift flange from pressure housing until seal is broken. The jacking screws can be used to "push" the flange from the pressure housing and then can be removed or left in the end flange.
- 7. Remove any excess moisture from flange—can seal area.
- 8. Work end flange out of pressure housing and remove any residual moisture. Remove the gray foam spacer and the neoprene insulator.
- 9. The battery pack is connected to the processor boards by a six-pin Molex connector: do NOT pull too hard or far on the battery pack or it will come unplugged and the unit returned to WET Labs.
- 10. Gently pull the white cord at the loop to remove the battery pack from the pressure housing.
- 11. Remove the black plastic protectors from the ends of the long screws securing the batteries.
- 12. Loosen and remove the screws (3/16-in slotted driver).



4.2 Replacing End Flange and Batteries

- 1. Replace the batteries.
- 2. Re-install the screws:
 - Align the groove in each of the plates so the six-wire extension bundle will fit in it along its length.
 - Be careful not to cross-thread into the bottom end plate nor to over-tighten the screws.
 - If they are too tight, the fiber washers that act as separators between the batteries will flex.
 - Make sure there are equal amounts of screw threads protruding from the bottom end plate when they are secure. This will ensure the pack is straight and will fit into the pressure housing with no difficulty.
- 3. Re-install the black plastic protective covers on the ends of the screws.
- 4. Remove and check the pressure housing O-ring for nicks or tears. Replace if necessary. Before re-installing, apply a light coat of vacuum grease on the O-ring.
- 5. Carefully replace the battery pack in the pressure housing. Place the neoprene insulator on the battery assembly and lay the white cord on the top.
- 6. Plug in the two-pin, then the six-pin Molex connectors. Sensor operation can now be tested if desired.
- 7. Align the hole in the end flange (NOT the jack screw holes) with the white dowel pin. While coiling the six wire bundle and making sure none are pinched between the end flange and the pressure housing, position the flange on the housing. Leave space to reinsert the gray foam spacer, making sure the cut-out accommodates the vent plug screw
- 8. Push the end flange all the way on to the pressure housing, making sure no wires are pinched. Be sure the vent plug does not pop up. If it does, you'll need to re-position the foam spacer.
- 9. Re-insert the monofilament.



4.3 Checking Vent Plug

If there is fouling on the vent plug, it should be cleaned and the two 010 O-rings replaced. Otherwise, this mechanism should be maintenance-free.

WARNING!

The pressure housing is made of plastic material that scratches easily. Do not let the screwdriver slip and scratch the can when removing or replacing the vent plug. Use a toothpick (something softer than the plastic) to remove the O-rings from the vent plug.

- 1. Pull vent plug out about half way; hold plug while unscrewing the truss screw. When screw is removed, pull vent plug from end flange.
- 2. "Pinch" bottom O-ring around vent plug to form a small gap you can work a toothpick into. Use the toothpick to help roll the bottom O-ring off the plug.
- 3. Perform the same procedure with the top O-ring.
- 4. Clean the vent plug and vent plug hole using a dry lint-free tissue or cotton swab.
- 5. Lightly coat two undamaged or new O-rings with silicon grease. Install the top O-ring (nearest to large end of plug) first, then the bottom one.
- 6. Insert vent plug into its hole in the end flange and hold it while inserting the truss screw. Rotate the vent plug to begin tightening the screw. Finish tightening using a screwdriver, being careful not to overtighten truss screw.

Note

A portion of the truss screw head has been removed to allow for venting in case of pressure buildup.



5. Data Analysis

Raw data from the BB is output as counts from the sensor, ranging from 0 to 4121. After the sensor is calibrated (i.e., subtracting the dark offset and multiplying by scaling factor—see Section 6), this data is now in the meaningful form of volume scattering coefficients, $\beta(\theta,\lambda)$ with units of m⁻¹ sr⁻¹, where θ is angle and λ is wavelength. The ECO host program will automatically perform the necessary calculations. Refer to the ECOView User's Guide for details of data collection.

5.1 Data Corrections

Attenuation coupling—For the population of photons scattered within the remote sample volume in front of the sensor face, there is attenuation along the path from the light source to the sample volume to the detector. This results in the scattering measurements being underestimates of the true volume scattering in the hydrosol. Corrected volume scattering coefficients can be obtained by accounting for the effect of attenuation along an average pathlength. This average pathlength was numerically solved in the weighting function determinations developed by Dr. Ron Zaneveld that are used in the calibration procedures.

Since the calibration of the *ECO*-VSF uses microspherical scatterers, the component of attenuation that can be attributed to scattering is incorporated into the scaling factor, i.e., the calibration itself. Thus, only absorption of the incident beam needs to be included in the correction.

The dependence on absorption, a, is determined as follows, where the measured scattering function at a given value of a, beta_meas(angle, a), is corrected to the value for $a = 0 \text{ m}^{-1}$, beta_corr(117°, a=0):

 $beta_corr(117^\circ, a=0) = beta_meas(117^\circ, a) exp(0.0391a)$

Absorption can be measured with an ac-9 device. For each ECO-BB wavelength, the matching absorption coefficient must be used from the ac-9. Because the ECO-BB incorporates short pathlengths and relatively small scattering volumes in its measurements, this attenuation error is typically small, about 4 percent at $a = 1 \text{ m}^{-1}$.

Temperature correction—Output from an LED reference detector is provided, which gives an indication of relative LED intensity during operation. Work is presently under way to incorporate this signal as an ongoing correction for measurements. Largest expected deviations in the calibration coefficients are about 10 percent in the temperature range 0–28 degrees C. Note that these errors become more pronounced for very clear waters. If the instrument is planned for use in clear water environments at the ends of this temperature range, it is recommended that a request be made for calibration data to be collected as close to the expected environmental temperature as possible.



5.2 Derived Parameters

5.2.1 Volume Scattering of Particles

The corrected volume scattering of particles, $\beta(117^{\circ},\lambda)$ values represent total volume scattering, i.e., scattering from particles and molecular scattering from water. To obtain the volume scattering of particles only, subtract the volume scattering of water, $\beta_w(117^{\circ},\lambda)$:

$$\beta_p(117^\circ,\lambda) = \beta(117^\circ,\lambda) - \beta_w(117^\circ,\lambda)$$

where $\beta_w(117^{\circ},\lambda)$ is obtained from the relationship (from Morel 1974):

$$\beta_{\rm w}(\theta,\lambda)=1.38(\lambda/500{\rm nm})^{-4.32}(1+0.3{\rm S}/37)10^{-4}(1+\cos^2\theta(1-\delta)/(1+\delta)){\rm m}^{-1}{\rm sr}^{-1},\ \delta=0.09$$

where S is salinity.

For total scattering of pure water,

$$b_{\rm w}(\lambda) = 0.0022533 \, (\lambda/500 \, {\rm nm})^{-4.23}$$
.

For total scattering of seawater (35–39 ppt),

$$b_{sw}(\lambda) = 0.0029308 (\lambda/500nm)^{-4.24}$$
.

For backscattering by water, divide b_w or b_{sw} by 2. The units for the b coefficients are (10^{-4} m^{-1}) .

5.2.2 Backscattering Coefficients

Particulate backscattering coefficients, $b_{bp}(\lambda)$ with units of m⁻¹, can be determined through estimation from the single measurement of $\beta_p(117^{\circ}, \lambda)$ using an X factor:

$$b_{bp} = 2\pi \times \beta_p(117^\circ)$$

From measurements of the volume scattering function with high angular resolution in a diversity of water types, Boss and Pegau (2001) have determined X to be **1.1** (Boss, E., and S. Pegau, 2001. The relationship of scattering in an angle in the back direction to the backscattering coefficient, *Applied Optics*). This factor estimates b_{bp} with an estimated uncertainty of 4 percent. The conversion can be used for $\beta(117^{\circ})$ measurements made at any visible wavelength.

To compute total backscattering coefficients, $b_b(\lambda)$ with units of m⁻¹, the backscattering from pure water, $b_{bw}(\lambda)$ (see Table above), needs to be added to $b_{bp}(\lambda)$:

$$b_b(\lambda) = b_{bp}(\lambda) + b_{bw}(\lambda).$$



6. Testing and Calibration

Prior to shipment, each *ECO* is tested and calibrated to ensure that it meets the instrument's stated specifications. The *ECO*-BB is typically configured for a measurement range of 0–5 m⁻¹ (red), and 0–10 m⁻¹ (blue or green). This is done at WET Labs by setting several gain settings inside the instrument and running a pure water blank to determine the zero voltage offset and to ensure that the dynamic range covers the measurement range of interest. As is the case with other scattering meters, a detailed calibration must be done by the user to determine the actual zero point and scale factor for his/her particular use.

6.1 Testing

When the instrument is completely assembled, it goes through the tests below to ensure performance.

6.1.1 Pure Water Blank

Pure, de-ionized water is used to set the "zero" level of the scattering meter. This zero level is set for 50 counts (+/-15) on all instruments.

6.1.2 Pressure

To ensure the integrity of the housing and seals, *ECOs* are subjected to a wet hyperbaric test before final testing. The testing chamber applies a water pressure of at least 50 PSI. The rated depth of the *ECO*-BB is 600 meters.

6.1.3 Mechanical Stability

Before final testing, the *ECO* is subjected to a mechanical stability test. This involves subjecting the unit to mild vibration and shock. Proper instrument functionality is verified afterwards.

6.1.4 Electronic Stability

This value is computed by collecting a sample once every five seconds for twelve hours, or more. After the data is collected, the standard deviation of this set is calculated and then divided by the number of hours the test has run. The stability value must be less than 2.0 mV/hour.

6.1.5 Resolution

Resolution is computed from a standard deviation over 60 samples, collected at one-second intervals for one minute. The standard deviation is calculated on the 60 samples, and the result is the published resolution on the calibration sheet. The calculated standard deviation value must be below 3 counts.

6.1.6 Voltage and Current Range Verification

To verify that the *ECO* operates over the entire specified voltage range (7–15V), a voltage-sweep test is performed. *ECO* is operated over the entire voltage range, and the current and operation is observed. The current must remain constant at approximately 85 mA over the entire voltage range.



6.2 Calibration

Each meter ships with a calibration sheet that provides instrument-specific calibration information, derived from the steps below.

- 1. For a given scattering centroid angle (θc), compute the weighting function W($\theta,\theta c$), by numerical integration of sample volume elements according to the sensor geometry.
- 2. Determine scattering phase functions, $\beta(\theta, \lambda)/b(\lambda)$, for the polystyrene bead microsphere calibration particles by weighting volume scattering functions computed from Mie theory according to the known size distribution of the polystyrene bead microsphere polydispersion and normalizing to total scattering.
- 3. By convolving $W(\theta, \theta c)$ with $\beta(\theta, \lambda)/b(\lambda)$, compute the normalized volume scattering coefficient for each measurement angle, $\beta(\theta, \lambda)/b(\lambda)$, with units of sr $^{-1}$ $\beta(\theta c)/b$ for 2.00-micron diameter polystyrene bead microspheres.
- 4. Experimentally obtain raw scattering counts simultaneously with attenuation coefficients (C_p, using an ac-9) for a concentration series of the polystyrene bead microsphere polydispersion. Absorption by the calibration particles is assumed negligible.
- 5. Obtain b/counts from the slope of a linear regression between Cp (equivalent to b for the beads) and counts.
- 6. Multiplying the experimental b/counts by the theoretical $\beta(\theta c)$ /b yields the calibration scaling factor, SF.
- 7. To obtain $\beta(\theta c)$, subtract the dark counts from the raw counts measured, then multiply by SF.
- 8. This test also provides a measure of the inherent opto-electronic noise level of the instrument. A standard deviation from the average number of counts on a 1 minute data file is taken. This is translated into the resolution of $\beta(\theta c)$ (minimum detectable signal change) in units of m^{-1} sr⁻¹.

Definitions of Terms

β: phase function b: total scattering coefficient

θ: angle
 W: weighting function
 C: centroid angle
 λ: wavelength
 SE: Scaling Factor

Cp: particulate attenuation coefficient m⁻¹: per meter SF: Scaling Factor sr⁻¹: per steradian



7. Terminal Communications

As an alternative to the ECOView Host software, *ECO* sensors can be controlled from a terminal emulator or customer-supplied interface software. This section outlines hardware requirements and low-level interface commands for this type of operation.

7.1 Interface Specifications

baud rate: 19200
data bits: 8
parity: none

• stop bits: 1 • flow control: none

7.2 Command List

Command	Parameters passed	Description	
!!!!!	none	Stops data collection; allows user to input setup parameters. Note that if the meter is in a sleep state, the power must be turned off for a minute, then powered on while the "!" key is held down for several seconds. If this does not "wake" the meter, refer to the ECOView user's guide Operation Tip to "wake" a meter in a low power sleep state to enable inputting setup parameters.	
\$asv	1, 2, or 4	Analog scaling value. Counts will be divided by this for analog output: a value of 4 will make the analog output cover the whole output range; 2 will cover half, and 1 will cover only the bottom fourth of the 14-bit count range (fluorometers only).	
\$ave	single number, 1 to 65535	Number of measurements for each reported value	
\$clk	24hr format time, hhmmss	Sets the time in the Real Time Clock	
\$dat	date, format ddmmyy	Sets the date in the Real Time Clock	
\$emc	none	Erases the Atmel memory chip, displays menu when done	
\$get	none	Reads data out of Atmel memory chip. Prints "etx" when completed.	
\$int	24hr format time, hhmmss	Time interval between packets in a set	
\$mnu	none	Prints the menu, including time and date	
\$pkt	single number, 0 to 65535	Number of individual measurements in each packet	
\$rec	1 (on) or 0 (off)	Enables or disables recording data to Atmel memory chip	
\$rls	none	Reloads settings from flash	
\$run	none	Executes the current settings	
\$set	single number, 0 to 65535	Number of packets in a set	
\$sto	none	Stores current settings to internal flash	
\$ugl	0 to 255	μg/l conversion value (calculates slope x 10,000). Fluorometer only.	



8. Device Files

The ECOView host program requires a device file to provide engineering unit outputs for any of its measurements. Except for the first line in the device file, all lines of information in the device file that do not conform to one of the descriptor headers will be ignored. Every ECOView device file has three required elements.

8.1 Plot Header

The first line in the device file is used as the plot header for the ECOView plots.

8.2 Column Count Specification

The Column Count Specification identifies how many columns of data to expect. It follows the format "Column=n." The Column Count Specification must be present before any of the Column Descriptions are listed.

8.3 Column Description

Every column in the ECO meter's output must have a corresponding Column Description in the device file. The following notation is used in identifying the elements of each Column Description.

x =the column number, starting with 1 as the 1^{st} column

sc = scale

dc = dark count: meter output in air with optics head taped

off = clean water offset, meter output in clean water

mw = wavelength measured by the sensor

dw = display wavelength—color to plot the BB data in

v = measured volts dc

Valid Column Descriptions are listed in the subsections below.

8.3.1 Scattering Measurements

Lambda=x sc off mw dw Scatter sensor column

8.3.2 Miscellaneous

Date=x DD/MM/YY Time=x HH:MM:SS

REF=x Reference Counts—Currently not used by ECOView

N/U=x The column is Not Used

There are several defaulted parameters that ECOView uses in the scatter calculations for the BB meters. These parameters are (a) salinity; (b) water type, fresh or sea water; (c) Chi; and (d) theta, the measurement angle. The user may change these using the following device file elements (the values shown are the defaults).



Salinity=32 32 ppt

Water=Sea Meter is assumed to be in salt water (Use "Pure" for fresh water)

XFactor=1.1 X Factor Correction Value Theta=117 Backscattering angle

8.4 Sample Device File

Below is the standard device file for an ECO BB at 532 nm.

```
ECO BBS-019G
Created on: 10/24/02
Columns=5
Date=1
Time=2
REF=3
Lambda=4 9.056e-06 67.1 532 532
N/U=5
```

8.5 Sample Output File


Below is a sample output file for a BB. From left to right, columns describe:

- 1. Date (MM/DD/YY)
- 2. Time (HH:MM:SS)
- 3. Scattering reference
- 4. Scattering signal
- 5. Thermistor (Note that if your sensor has the optional temperature sensor, the output in the last column will have an extra digit. Temperature is output in degrees C in ECOView.)

```
02/19/03
          13:56:28
                      1752 1211
                                 541
02/19/03
          13:56:29 1739 1225
                                 540
02/19/03 13:56:30 1732 1230 540
02/19/03 13:56:31 1728 1200 540
02/19/03 13:56:32 1724 1191
                                 539
02/19/03 13:56:33 1722 1186 539
02/19/03 13:56:33 1720 1180 538
02/19/03 13:56:34 1718 1181 539
02/19/03 13:56:35 1717 1181 538
02/19/03 13:56:36 1715 1184 538
02/19/03 13:56:37 1714 1173 538
02/19/03 13:56:38 1713 1181
                                 538
          13:56:39 1713 1182
02/19/03
                                 538
        13:56:40
                     1712 1187
02/19/03
                                 538
02/19/03 13:56:41 1711 1171
                                 538
02/19/03 13:56:42 1711 1177 538
02/19/03 13:56:43 1710 1177 538
```



Appendix A: Mounting Bracket Drawing

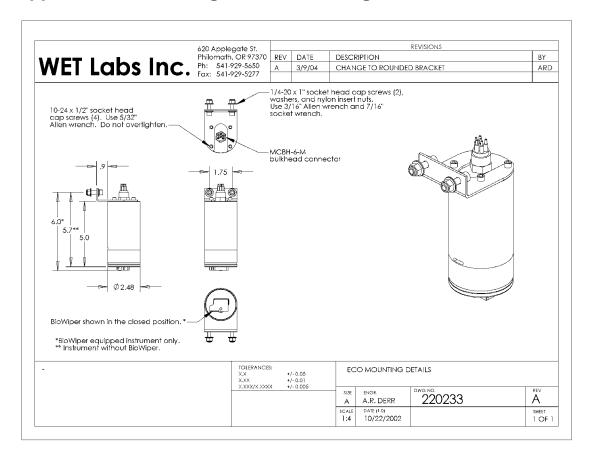



Revision History

Revision	Date	Revision Description	Originator
Α	10/16/02	New document (DCR 242)	W. Strubhar, D. Whiteman
В	10/23/02	Add mounting bracket hardware description (DCR	A. Derr
		251)	
С	11/12/02	Add analog capability for (RT) models (DCR 254)	I. Walsh
D	2/10/03	Delete lithium battery warning (DCR 272)	D. Whiteman
E	2/24/03	Change "shutter" to "bio-wiper™" (DCR 280)	H. Van Zee
F	3/3/03	Add Terminal Communications section (DCR 283)	I. Walsh
G	4/14/03	Add stop command to terminal communications (DCR 292)	W. Strubhar
Н	5/29/03	Clarify equations in section 5.2.1 (DCR 303)	M. Twardowski
Ι	8/6/03	Add to deliverables list, correct references in Data Analysis, update device files (DCR 321)	H. Van Zee
J	9/8/03	Add Scaling Factor derivation to Calibration Section (DCR 332)	D. Hankins, H. Van Zee, I. Walsh
K	11/24/03	Modify explanation for stop data collection command (DCR 342)	W. Strubhar
L	11/25/03	Update specifications (DCR 338)	I. Walsh
L1	2/3/04	Add device file change for optional pressure/temperature sensor	I. Walsh
М	2/5/04	Correct salinity value (DCR 365)	I. Walsh, D. Romanko
N	2/17/04	Update to neoprene bio-wiper blade (DCR 367)	A. Derr, I. Walsh
0	3/10/04	Add new test cable description, operational description, mounting diagram (DCR 381)	A. Derr, D. Whiteman
Р	5/11/04	Remove pin 6 from warning in section 1 (DCR 390)	I. Walsh