

# ***ECO* Fluorometer**

*ECO* FL

## User's Guide

The user's guide is an evolving document. If you find sections that are unclear, or missing information, please let us know. Please check our website periodically for updates.

WET Labs, Inc.  
P.O. Box 518  
Philomath, OR 97370  
541-929-5650  
fax: 541-929-5277  
wetlabs@wetlabs.com  
www.wetlabs.com



## Attention!

### **Return Policy for Instruments with Anti-fouling Treatment**

WET Labs cannot accept instruments for servicing or repair that are treated with anti-fouling compound(s). This includes but is not limited to tri-butyl tin (TBT), marine anti-fouling paint, ablative coatings, etc.

Please ensure any anti-fouling treatment has been removed prior to returning instruments to WET Labs for service or repair.



## ***ECO Sensor Warranty***

This unit is guaranteed against defects in materials and workmanship for a period of one year after the original date of purchase. WET Labs will supply all replacement parts and labor and pay for return via 3<sup>rd</sup> day air shipping in honoring this warranty. This warranty is considered void if the factory determines that the unit was subjected to abuse or neglect beyond the normal wear and tear of field deployment, or in the event the pressure cans have been opened by the customer (this does not apply to pressure cans on battery-supplied units). The customer should call for a Return Manufacturer's Authorization (RMA) before returning the instrument to the factory and is responsible for shipping costs to WET Labs. WET Labs is not responsible for shipping damage done during the return shipment. WET Labs assumes no liability for equipment damage, personal injury or loss of data resulting from use of this instrument, except for that stated in this warranty.



## Table of Contents

<b>1.</b>	<b>Overview</b> .....	<b>1</b>
1.1	Specifications.....	1
1.2	Connectors.....	3
1.3	Test Cable.....	4
1.4	Delivered Items.....	5
1.5	Bio-wiper™.....	5
1.6	Batteries.....	5
<b>2.</b>	<b>Theory of Operation</b> .....	<b>6</b>
<b>3.</b>	<b>Instrument Operation</b> .....	<b>7</b>
3.1	Initial Checkout.....	7
3.2	Operating the Sensor for Data Output.....	7
3.3	Deployment.....	8
3.4	Upkeep and Maintenance.....	8
3.5	<i>Bio-wiper™</i> Operation.....	9
<b>4.</b>	<b>FLB and FLSB: Using Internal Batteries</b> .....	<b>11</b>
4.1	Removing End Flange and Batteries.....	11
4.2	Replacing End Flange and Batteries.....	12
4.3	Checking Vent Plug.....	13
<b>5.</b>	<b>Data Analysis</b> .....	<b>14</b>
5.1	Analog Response.....	14
5.2	Digital Response.....	14
<b>6.</b>	<b>Characterization and Testing</b> .....	<b>15</b>
6.1	Testing.....	15
<b>7.</b>	<b>Terminal Communications</b> .....	<b>16</b>
7.1	Interface Specifications.....	16
7.2	Command List.....	16
<b>8.</b>	<b>Device Files</b> .....	<b>17</b>
8.1	Plot Header.....	17
8.2	Column Count Specification.....	17
8.3	Column Description.....	17
8.4	Sample Device Files.....	18
8.5	Sample Output File.....	19
<b>Appendix A: Mounting Bracket Drawing</b> .....		<b>20</b>



## 1. Overview

WET Labs offers a range of the *Environmental Characterization Optics (ECO)* series fluorometers for the following measurements: chlorophyll, Colored Dissolved Organic Matter, uranine, rhodamine, phycocyanin, and phycoerythrin. This section includes meter and connector specifications, delivered items and descriptions of features, including internal batteries and *bio-wiper™*.

### 1.1 Specifications

**FL(RT)**—Provides analog or RS-232 serial output with 4,000-count range. This unit provides continuous operation when powered.

**FL(RT)D**—Provides the capabilities of the FL(RT) with 6,000-meter depth rating.

**FL**—Provides the capabilities of the FL(RT) with periodic sampling.

**FLS**—Provides the capabilities of the FL with an integrated anti-fouling *bio-wiper™*.

**FLB**—Provides the capabilities of the FL with internal batteries for autonomous operation.

**FLSB**—Provides the capabilities of the FLS with internal batteries for autonomous operation.

	<b>FL(RT)</b>	<b>FL(RT)D</b>	<b>FL</b>	<b>FLS</b>	<b>FLB</b>	<b>FLSB</b>
<b>Mechanical</b>						
<i>Diameter</i>	2.48 in (6.3 cm)					
<i>Length</i>	5.0 in (12.7 cm)	7 in (17.8 cm)	5.0 in (12.7 cm)	5.25 in (13.3 cm)	10.0 in (25.4 cm)	10.25 in (26.0 cm)
<i>Weight (in air)</i>	0.9 lbs (0.4 kg)	2.86 lbs (1.3 kg)	0.9 lbs (0.4 kg)	1.1 lbs (0.5 kg)	2.1 lbs (0.96 kg)	2.1 lbs (0.96 kg)
<i>Weight (in water)</i>	0.05 lbs (0.02 kg)	1.66 lbs (0.75 kg)	0.05 lbs (0.02 kg)	0.19 lbs (0.08 kg)	0.3 lbs (0.14 kg)	0.3 lbs (0.14 kg)
<i>Pressure housing</i>	ABS	ABS	ABS	ABS	ABS	ABS
<b>Environmental</b>						
<i>Temperature range</i>	0–30 deg C					
<i>Depth rating</i>	600 m	6000 m	600 m	300 m	600 m	300 m
<i>Pressure/temperature sensor (optional)</i>	Y	Y	Y	Y	Y	Y
<b>Electrical</b>						
<i>Digital output resolution</i>	14 bit					
<i>Analog output signal</i>	0–5 V					
<i>Internal data logging</i>	N	N	Y	Y	Y	Y
<i>Internal batteries</i>	N	N	N	N	Y	Y
<i>Connector</i>	MCBH6M	MCBH6M	MCBH6M	MCBH6M	MCBH6M	MCBH6M
<i>Input voltage</i>	7–15 VDC					
<i>Current, typical</i>	80 mA					
<i>Current, sleep</i>	--	--	85 µA	85 µA	85 µA	85 µA
<i>Data memory</i>	--	--	1 MB (65,000 samples)			
<i>Sample rate</i>	to 8 Hz					
<i>RS-232 output</i>	19200 baud					
<i>Anti-fouling bio-wiper</i>	N	N	N	Y	N	Y
<i>Bio-wiper™ cycle</i>	-	-	-	110 mA	-	110 mA

## Optical Specifications for Fluorescence Meters

### **Chlorophyll-*a* (FL-CHL)**

Ex/Em: 470/695 nm • Sensitivity: 0.025 µg/l • Linearity: 99% R<sup>2</sup> • Range: 100 µg/l

### **Colored Dissolved Organic Matter (FL-CD)**

Ex/Em: 390/460 nm • Sensitivity: 0.025 ppb QS • Linearity: 99% R<sup>2</sup> • Range: 100 ppb

### **Uranine (fluorescein) (FL-UR)**

Ex/Em: 470/530 nm • Sensitivity: 1 ppb • Linearity: 99% R<sup>2</sup> • Range: 4000 ppb

### **Rhodamine**

Ex/Em: 540/570 nm • Sensitivity: 1 ppb • Linearity: 99% R<sup>2</sup> • Range: 4000 ppb

### **Phycoerythrin (FL-PE)**


Ex/Em: 540/570 nm • Sensitivity: 1 ppb • Linearity: 99% R<sup>2</sup> • Range: 4000 ppb

Other ranges available on request.

*Specifications subject to change without notice.*

## 1.2 Connectors

*ECO*-series digital fluorometers use a six-pin bulkhead connector. The pin functions for this connector are shown in Figure 1. Table 1 summarizes pin functions for the bulkhead connectors.

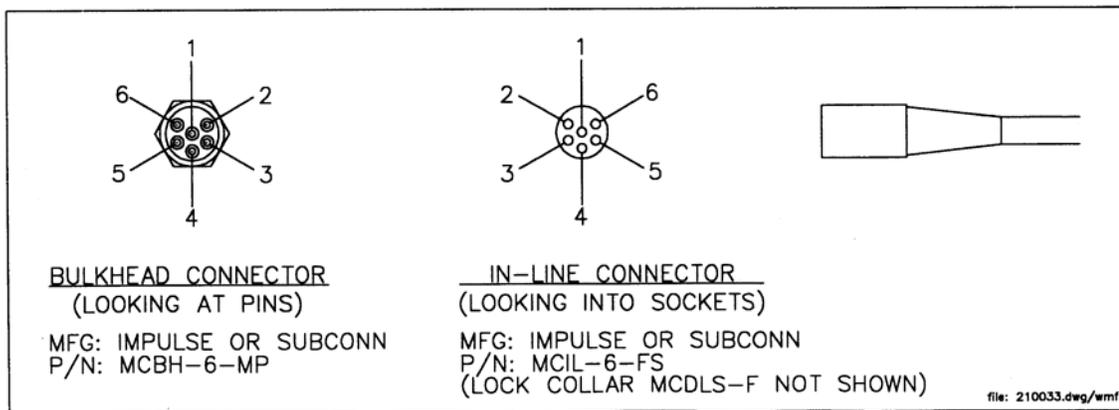

**Figure 1.** *ECO* FL connector schematic

**Table 1.** Pinout summary for *ECO* connectors

Pin (or Socket)	Function
1	Ground
2	RS-232 (RX)
3	Reserved
4	V in
5	RS-232 (TX)
6	Analog out


### WARNING

**If you are going to build or use a non-WET Labs-built cable, do not use the wire from pin 3 or the *ECO* meter will be damaged.**

Input power of 7–15 VDC is applied to pin 4. The power supply current returns through the common ground pin. The input power signal has a bi-directional filter. This prevents external power supply noise from entering into *ECO* FL, and also prevents internally generated noise from coupling out on to the external power supply wire. Data is sent out the serial output pin.

#### 1.2.1 *ECO* FLB, FLSB Connectors

*ECO* FLB and FLSB (units with internal batteries) have a second bulkhead connector that comes with a jumper plug to supply power to the unit. The pin functions for this connector are shown in Figure 2. Table 2 summarizes pin functions for the 3-socket bulkhead connector.

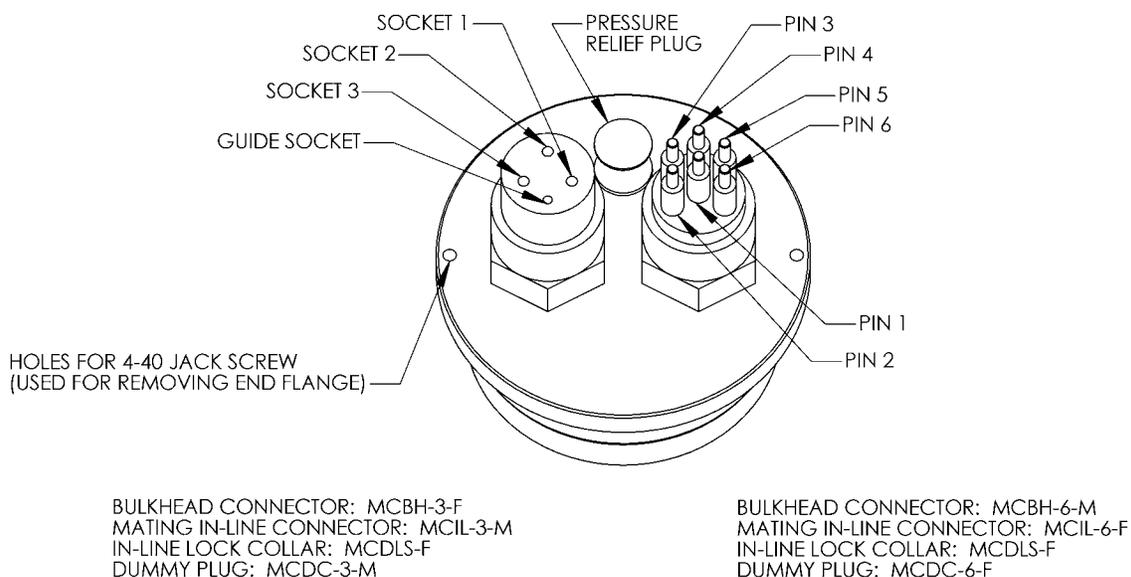

**Figure 2.** ECO FLB and FLSB connector schematic

**Table 2.** Pinout summary for ECO FLB/FLSB 3-socket connector

Pin (or Socket)	Function
1	V in
2	N/C
3	Battery out

### 1.3 Test Cable

A test cable is supplied with each unit. This cable includes four legs:

1. A power interface module provides power to the instrument from the connected 9 V battery.
2. An auxiliary analog out connector.
3. A DB-9 serial interface connector.
4. A six-socket in-line connector plugs into the sensor to provide power and obtain signal.

FLB and FLSB (internal battery units) are supplied with a jumper plug that provides power from the internal batteries for autonomous operation. (Power is supplied from pin 6 to pin 4.)

## 1.4 Delivered Items

The standard ECO delivery consists of the following:

- the instrument itself
- dummy plug with lock collar
- protective cover for optics
- test cable
- this user's guide
- ECOView user's guide
- ECOView host program and device files (on CD)
- instrument-specific calibration sheet
- FL(RT), FL, FLS only: stainless steel mounting bracket and hardware (See Appendix A for details)
- fluorescent stick for bench testing
- One 0.050-in. hex key for *bio-wiper*<sup>™</sup> removal (units with *bio-wiper*<sup>™</sup> only)
- spare parts kit (battery units only):
  - Two end flange O-rings (size 224) and two vent plug O-rings (size 010)
  - Two jacking screws for connector flange removal
  - One 3/32-in. hex key for jacking screws
  - Power plug for autonomous operation
  - Three pre-cut segments (7 inches) of 0.036-inch diameter monofilament for end flange
  - Three pre-cut segments (0.25 inches) of 0.094-inch diameter white nylon bar stock for replacing the white plastic dowel pin.

## 1.5 Bio-wiper<sup>™</sup>

The FLS and FLSB include an integrated non-contact anti-fouling *bio-wiper*<sup>™</sup> for use in extended deployments. This *bio-wiper*<sup>™</sup> can be manually controlled by a host controller package, or can perform autonomously as part of a pre-programmed sampling sequence upon instrument power-up. The rate of closure and opening is dependent upon both temperature and depth.

## 1.6 Batteries

The FLB and FLSB incorporate six 9-volt batteries as their internal power source. They can either use standard alkaline cells for a total capacity of approximately 1000 mA-hrs, or for longer deployments can use LiMnO<sub>2</sub> cells to achieve more than 2000 mA-hrs of operational capacity. Actual total usage time of the internal batteries is a function of several parameters. These include nominal water temperature, sequence timing, sample periods, and total deployment duration.

### **WARNING!**


**Pin 6 is always "hot." Be sure to keep the dummy plug on the FLB and FLSB when not in use.**

---

For even greater deployment capability contact WET Labs for information on external battery packs.

## 2. Theory of Operation

The *Environmental Characterization Optics*, or *ECO* miniature fluorometer allows the user to measure relative chlorophyll, CDOM, uranine, phycocyanin, or phycoerythrin concentrations by directly measuring the amount of fluorescence emission in a sample volume of water. The *ECO* uses an LED to provide the excitation source. An interference filter is used to reject the small amount of out-of-band light emitted by the LED. The light from the source enters the water volume at an angle of approximately 55–60 degrees with respect to the end face of the unit. Fluoresced light is received by a detector positioned where the acceptance angle forms a 140-degree intersection with the source beam. An interference filter is used to discriminate against the scattered excitation light.

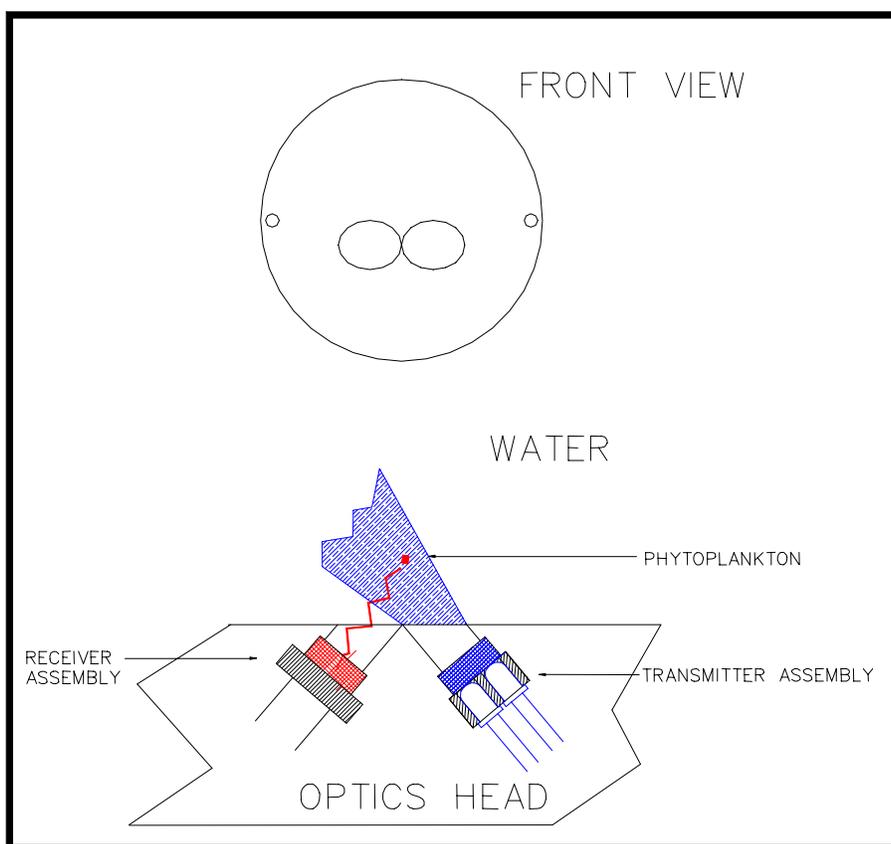

**Figure 3.** Optical configuration of *ECO* fluorometer

### 3. Instrument Operation

Please note that certain aspects of instrument operation are configuration-dependent. These are noted where applicable within the manual.

#### 3.1 Initial Checkout

Supplied from the factory, *ECOs* are configured to begin continuously sampling upon power-on. Electrical checkout of *ECO* is straightforward.

Connect the 6-socket connector on the test cable to the instrument to provide power to the LEDs and electronics (see Section 1 for a diagram of the pinouts of *ECO FL*). Connect the battery leads on the test cable to the 9V battery supplied with the meter. Light should emanate from the meter.

##### 3.1.1 Analog Option

Connect a digital multimeter (DMM) to the auxiliary leg of the test cable: the center of the RCA connector provides analog out signal and the outside provides ground. With the sensor face clean and dry the instrument should read approximately 0.050–0.095 VDC. The analog signal will saturate at 5 volts.

#### 3.2 Operating the Sensor for Data Output

##### Note

*ECO* scattering meters are sensitive to AC light. Before making measurement, turn AC lighting off.

---

1. Connect the 6-socket connector to the instrument to provide power to the LEDs and electronics. Connect the DB-9 connector to a computer with the ECOView host program installed on it.

##### WARNING!

**Always use a regulated power supply to provide power to ECO sensors if not using the 9V battery provided with the test cable: power spikes may damage the meter.**

2. Start ECOView. Select the appropriate COM Port and Device File. Supply power to the meter, then click on the **Start Data** button. Output will appear in the Raw Data window. Place the flat of your hand in front of the sensor face and note that the signal will increase toward saturation (maximum value on characterization sheet) as your hand gets closer. When applying power to sensors with a *bio-wiper*<sup>TM</sup>, it will open and, depending on the settings, operate until you select **Stop Data** in ECOView (or input ! ! ! ! in a terminal program) The *bio-wiper*<sup>TM</sup> will close and the instrument will await the next command.

- 
3. If the sensor completes the requested samples (this is common for meters set up in moored applications), it will go into sleep mode, and the meter will not light when power is cycled. To “wake” the meter, click **Stop Data** five times at the rate of two times a second immediately upon supplying power. This interrupts the sensor, returning it to a “ready” state, awaiting commands.
  4. Check the settings for the ECO and change if necessary. ECOView factory settings for continuous operation:
    - Set Number of Samples = 0
    - Set Number of Cycles = 0.
  5. If the meter does not light after performing step 3, check the battery. Replace if necessary, perform steps 2 and 3 to verify communication. If it still does not light, contact WET Labs.

Refer to the ECOView User’s Guide for details about using the software.

### 3.3 Deployment

Once power is supplied to the ECO meter, the unit is ready for submersion and subsequent measurements. Some consideration should be given to the package orientation. Do not face the sensor directly into the sun or other bright lights. For best output signal integrity, locate the instrument away from significant EMI sources.

Other than these basic considerations, one only needs to make sure that the unit is securely mounted to whatever lowering frame is used and that the mounting brackets are not damaging the unit casing.

#### Note

FLB and FLSB: Always check vent seal plug for full insertion immediately prior to deployment.

### 3.4 Upkeep and Maintenance

The *ECO-FL* is compact device and its maintenance can be easily overlooked. However, it is a precision instrument and does require a minimum of routine upkeep. After each cast or exposure of the instrument to natural water, flush the instrument with clean fresh water, paying careful attention to the sensor face. Use soapy water to cut any grease or oil accumulation. Gently wipe clean with a soft cloth. The sensor face is composed of ABS plastic and optical epoxy and can easily be damaged or scratched. At the end of an experiment, the instrument should be rinsed thoroughly, air-dried and stored in a cool, dry place.

#### WARNING!

**Do not use acetone or other solvents to clean the sensor.**

### 3.5 *Bio-wiper*<sup>TM</sup> Operation

The *ECO*-FLS and -FLSB are provided with an anti-fouling *bio-wiper*<sup>TM</sup>. The *bio-wiper*<sup>TM</sup> extends the possible deployment duration by retarding biological growth on the instrument's optical surface. The *bio-wiper*<sup>TM</sup> covers the optical surface: 1) while the instrument is in "sleep" mode; 2) when it has completed the number of samples requested; and 3) when the user selects **Stop Data** in *ECOView* or types "!!!!" in a terminal program. When the meter wakes up, the optical surface is exposed by the *bio-wiper*'s<sup>TM</sup> counter-clockwise rotation.

If power is shut off in mid cycle, the *bio-wiper*<sup>TM</sup> will reinitialize to the beginning of the user-selected settings when power is applied again.


#### 3.5.1 *Bio-wiper*<sup>TM</sup> Cleaning and Maintenance

When not in active sample mode, the *bio-wiper*<sup>TM</sup> can be removed by using the factory-supplied 0.050 hex key to loosen the set screw that attaches the shutter to the instrument. Take care to ensure no unnecessary torque is placed on the shaft.

To clean, wash in soapy water, rinse and dry thoroughly. Note the condition of the copper on the instrument side of the shutter. It is normal for the copper *bio-wiper*<sup>TM</sup> to corrode and turn green, especially after the instrument has been removed from the water. This corrosion will slightly reduce the shutter's antifouling ability the next time it is deployed. For maximum antifouling capability:

1. Remove *bio-wiper*<sup>TM</sup>
2. Buff with a pad of green Scotch Brite<sup>®</sup> (or similar) until shiny
3. Re-install *bio-wiper*<sup>TM</sup>

When re-installing the *bio-wiper*<sup>TM</sup> on the instrument, the wiper blade must be properly flexed. To achieve the proper flex of the wiper, set the gap between the copper *bio-wiper*<sup>TM</sup> and the instrument face to 0.03 in. (0.8 mm). An improperly set gap will either fail to clean the face, or cause the motor to draw excessive current (Figure 4).

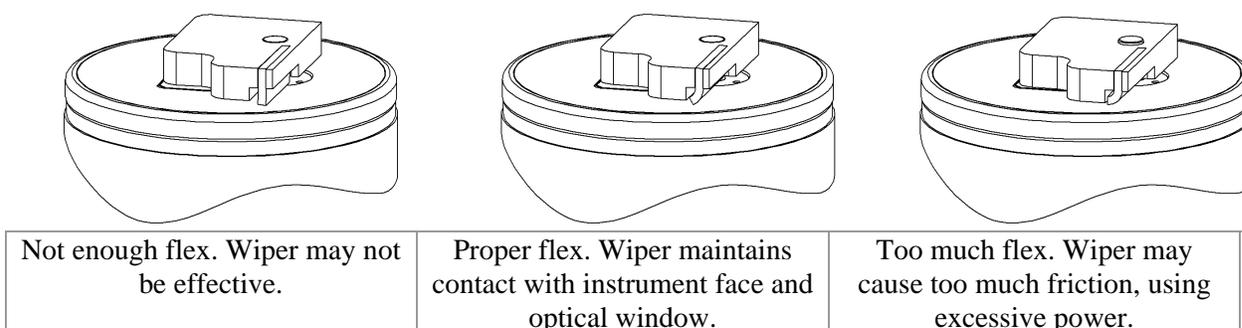

**Figure 4.** Adjusting *bio-wiper*<sup>TM</sup> for proper flex

To set this gap:

1. Fold a piece of paper in half, then in half again, then fold a third time, creasing the edges. It's now 8 sheets thick and about 0.03 in. thick.
2. Make sure the *bio-wiper*<sup>TM</sup> is in the closed position. You may have to run the instrument.
3. If it is not already loosened, loosen the set screw holding the *bio-wiper*<sup>TM</sup> and put the paper gage between the instrument face and the bio-wiper.
4. Push down on the *bio-wiper*<sup>TM</sup> and rotate it counter-clockwise so that the shutter is in the closed position.
5. Without letting the wiper spring up, tighten the set screw.
6. Run the instrument to verify operation

## 4. FLB and FLSB: Using Internal Batteries

ECO sensors powered with internal batteries can either run directly from the internal batteries or can operate from power supplied by an external DC power supply (7–15 volts). Internal-to-external source conversion is facilitated by a jumper plug that plugs into the unit’s bulkhead connector. When inserted, the plug forms a connection from the battery to the electronics power supply. By removing the plug, the instrument can be powered and communicate via a test or deployment cable. Setup conditions, instrument checkout, real-time operation, and data downloading are thus all achieved identically to the methods prescribed for the FL and FLS units.

### 4.1 Removing End Flange and Batteries

#### **WARNING!**

**Changing the batteries will require opening the pressure housing of the ECO sensor. Only people qualified to service underwater oceanographic instrumentation should perform this procedure. If this procedure is performed improperly, it could result in catastrophic instrument failure due to flooding or in personal injury or death due to abnormal internal pressure as a result of flooding.**

**WET Labs Inc. disclaims all product liability from the use or servicing of this equipment. WET Labs Inc. has no way of controlling the use of this equipment or of choosing qualified personnel to operate it, and therefore cannot take steps to comply with laws pertaining to product liability, including laws that impose a duty to warn the user of any dangers involved with the operation and maintenance of this equipment.**

**Therefore, acceptance of this equipment by the customer shall be conclusively deemed to include a covenant by the customer to defend and hold WET Labs Inc. harmless from all product liability claims arising from the use and servicing of this equipment. Flooded instruments will be covered by WET Labs Inc. warranties at the discretion of WET Labs, Inc.**

---

1. Make sure the instrument is thoroughly dry.
2. Remove the dummy plugs.
3. With connector end flange pointed downwards away from face, release seal from vent plug.
4. Remove moisture from vent plug area.
5. Using needle nose pliers, remove filament from end flange.
6. Lift flange from pressure housing until seal is broken. The jacking screws can be used to “push” the flange from the pressure housing and then can be removed or left in the end flange.
7. Remove any excess moisture from flange–can seal area.
8. Work end flange out of pressure housing and remove any residual moisture. Remove the gray foam spacer and the neoprene insulator.

9. The battery pack is connected to the processor boards by a six-pin Molex connector: do NOT pull too hard or far on the battery pack or it will come unplugged and the unit returned to WET Labs.
10. Gently pull the white cord at the loop to remove the battery pack from the pressure housing.
11. Remove the black plastic protectors from the ends of the long screws securing the batteries.
12. Loosen and remove the screws (3/16-in slotted driver).

#### **4.2 Replacing End Flange and Batteries**

1. Replace the batteries.
2. Re-install the screws:
  - Align the groove in each of the plates so the six-wire extension bundle will fit in it along its length.
  - Be careful not to cross-thread into the bottom end plate nor to over-tighten the screws.
  - If they are too tight, the fiber washers that act as separators between the batteries will flex.
  - Make sure there are equal amounts of screw threads protruding from the bottom end plate when they are secure. This will ensure the pack is straight and will fit into the pressure housing with no difficulty.
3. Re-install the black plastic protective covers on the ends of the screws.
4. Remove and check the pressure housing O-ring for nicks or tears. Replace if necessary. Before re-installing, apply a light coat of vacuum grease on the O-ring.
5. Carefully replace the battery pack in the pressure housing. Place the neoprene insulator on the battery assembly and lay the white cord on the top.
6. Plug in the two-pin, then the six-pin Molex connectors. Sensor operation can now be tested if desired.
7. Align the hole in the end flange (NOT the jack screw holes) with the white dowel pin. While coiling the six wire bundle and making sure none are pinched between the end flange and the pressure housing, position the flange on the housing. Leave space to re-insert the gray foam spacer, making sure the cut-out accommodates the vent plug screw.
8. Push the end flange all the way on to the pressure housing, making sure no wires are pinched. Be sure the vent plug does not pop up. If it does, you'll need to re-position the foam spacer.
9. Re-insert the monofilament.

### **4.3 Checking Vent Plug**

If there is fouling on the vent plug, it should be cleaned and the two 010 O-rings replaced. Otherwise, this mechanism should be maintenance-free.

#### **WARNING!**

**The pressure housing is made of plastic material that scratches easily. Do not let the screwdriver slip and scratch the can when removing or replacing the vent plug. Use a toothpick (something softer than the plastic) to remove the O-rings from the vent plug.**

---

1. Pull vent plug out about half way; hold plug while unscrewing the truss screw. When screw is removed, pull vent plug from end flange.
2. “Pinch” bottom O-ring around vent plug to form a small gap you can work a toothpick into. Use the toothpick to help roll the bottom O-ring off the plug.
3. Perform the same procedure with the top O-ring.
4. Clean the vent plug and vent plug hole using a dry lint-free tissue or cotton swab.
5. Lightly coat two undamaged or new O-rings with silicon grease. Install the top O-ring (nearest to large end of plug) first, then the bottom one.
6. Insert vent plug into its hole in the end flange and hold it while inserting the truss screw. Rotate the vent plug to begin tightening the screw. Finish tightening using a screwdriver, being careful not to overtighten truss screw.

#### **Note**

A portion of the truss screw head has been removed to allow for venting in case of pressure buildup.

---

## 5. Data Analysis

Data from the *ECO* fluorometer, whether digital or analog, represents raw output from the sensor. Applying linear scaling constants, this data can be expressed in meaningful forms of fluorescence.

### 5.1 Analog Response

The *ECO*-FL response is linear over the measurement range provided. Because of the varied environments in which each user will work, it is important to do calibrations using similar seawater as you expect to encounter *in situ*. Please refer to characterization section for further details. This will provide an accurate blank, equivalent phytoplankton types and similar physiological conditions for calculating the scale factor, thereby providing an accurate and meaningful calibration. Once a zero point has been determined and a scale factor established, the conversion of DC volts to chlorophyll, CDOM, uranine, phycocyanin, or phycoerythrin concentration is straightforward using the equation:

$$[\text{XX}]_{\text{sample}} = (V_{\text{sample}} - V_{\text{blank}}) * \text{Scale Factor}$$

where  $[\text{XX}]_{\text{sample}}$  = Concentration of a sample of interest ( $\mu\text{g/l}$  or  $\text{ppb}$ )  
 $V_{\text{sample}}$  = voltage output when measuring a sample of interest (VDC)  
 $V_{\text{blank}}$  = measured signal for a sea water blank (VDC)  
 Scale factor = multiplier in  $\mu\text{g/l}$ -volts or  $\text{ppb}$ -volts

A scale factor is then applied to the analog output signal to provide the direct conversion of the analog output voltage to chlorophyll concentration.

A scale factor is supplied from the factory. While this constant can be used to obtain approximate values, field calibration is highly recommended.

### 5.2 Digital Response

Digital data is processed in a similar fashion to analog data. Scaling is linear, and obtaining a “calibrated” output simply involves subtracting a digital offset value and multiplying the difference by the instrument scaling factor.

$$[\text{XX}]_{\text{sample}} = (C_{\text{sample}} - C_{\text{blank}}) * \text{Scale Factor}$$

where  $[\text{XX}]_{\text{sample}}$  = Concentration of a sample of interest ( $\mu\text{g/l}$  or  $\text{ppb}$ )  
 $C_{\text{sample}}$  = Raw counts output when measuring a sample of interest  
 $C_{\text{blank}}$  = Measured signal in raw counts for a sea water blank  
 Scale factor = multiplier in  $\mu\text{g/l}$ -counts or  $\text{ppb}$ -counts.

## 6. Characterization and Testing

Prior to shipment, each *ECO* is characterized to ensure that it meets the instrument's specifications. Gain selection is done at WET Labs by setting several gain settings inside the instrument, and running a chlorophyll (or proxy) dilution series to determine the zero voltage offset and to ensure that the dynamic range covers the measurement range of interest. The dilution series also establishes the linearity of the instrument's response.

### 6.1 Testing

When the instrument is completely assembled, it goes through the tests below to ensure performance.

#### 6.1.1 Pure Water Blank

Pure, de-ionized water is used to set the "zero" level of the meter. This zero level is set for 50 counts (+/-15) on all models.

#### 6.1.2 Pressure

To ensure the integrity of the housing and seals, ECOs are subjected to a wet hyperbaric test before final testing. The testing chamber applies a water pressure of at least 50 PSI.

#### 6.1.3 Mechanical Stability

Before final testing, the *ECO-FL* meters are subjected to a mechanical stability test. This involves subjecting the unit to mild vibration and shock. Proper instrument functionality is verified afterwards.

#### 6.1.4 Electronic Stability

This value is computed by collecting a sample once every 5 seconds for twelve hours or more. After the data is collected, the standard deviation of this set is calculated and divided by the number of hours the test ran. The stability value must be less than 2.0 mV/Hour.

#### 6.1.5 Noise

The noise "figure" is computed from a standard deviation over 60 samples. These samples are collected at one-second intervals for one minute. A standard deviation is then performed on the 60 samples, and the result is the published noise on the calibration form. The calculated noise must be below 2 mV.

#### 6.1.6 Voltage and Current Range Verification

To verify that the *ECO* operates over the entire specified voltage range (7–15 V), a voltage-sweep test is performed. ECO is operated over the entire voltage range, and the current and operation is observed. The current must remain constant at approximately 85 mA over the entire voltage range.

## 7. Terminal Communications

As an alternative to the ECOView host software, *ECO* sensors can be controlled from a terminal emulator or customer-supplied interface software. This section outlines hardware requirements and low-level interface commands for this type of operation.

### 7.1 Interface Specifications

- baud rate: 19200
- data bits: 8
- parity: none
- stop bits: 1
- flow control: none

### 7.2 Command List

Command	Parameters passed	Description
!!!!	none	Stops data collection; allows user to input setup parameters. Note that if the meter is in a sleep state, the power must be turned off for a minute, then powered on while the “!” key is held down for several seconds. If this does not “wake” the meter, refer to the ECOView user’s guide Operation Tip to “wake” a meter in a low power sleep state to enable inputting setup parameters.
\$asv	1, 2, or 4	Analog scaling value. Counts will be divided by this for analog output: a value of 4 will make the analog output cover the whole output range; 2 will cover half, and 1 will cover only the bottom fourth of the 14-bit count range (fluorometers only).
\$ave	single number, 1 to 65535	Number of measurements for each reported value
\$clk	24hr format time, hhmmss	Sets the time in the Real Time Clock
\$dat	date, format ddmmyy	Sets the date in the Real Time Clock
\$emc	none	Erases the Atmel memory chip, displays menu when done
\$get	none	Reads data out of Atmel memory chip. Prints "etx" when completed.
\$int	24hr format time, hhmmss	Time interval between packets in a set
\$mnu	none	Prints the menu, including time and date
\$pkt	single number, 0 to 65535	Number of individual measurements in each packet
\$rec	1 (on) or 0 (off)	Enables or disables recording data to Atmel memory chip
\$rls	none	Reloads settings from flash
\$run	none	Executes the current settings
\$set	single number, 0 to 65535	Number of packets in a set
\$sto	none	Stores current settings to internal flash
\$ugl	0 to 255	µg/l conversion value (calculates slope x 10,000). Fluorometer only.

## 8. Device Files

The ECOView host program requires a device file to provide engineering unit outputs for any of its measurements. Except for the first line in the device file, all lines of information in the device file that do not conform to one of the descriptor headers will be ignored. Every ECOView device file has three required elements.

### 8.1 Plot Header

The first line in the device file is used as the plot header for the ECOView Plots.

### 8.2 Column Count Specification

The Column Count Specification identifies how many columns of data to expect. It follows the format “Column=n.” The Column Count Specification must be present before any of the Column Descriptions are listed.

### 8.3 Column Description

Every column in the ECO meter’s output must have a corresponding Column Description in the device file. The following notation is used in identifying the elements of each Column Description.

- x = the column number, starting with 1 as the 1<sup>st</sup> column
- sc = scale
- dc = dark count: meter output in air with optics head taped
- off = clean water offset, meter output in clean water
- mw = measurement wavelength—wavelength used by the sensor for its measurement
- dw = display wavelength—wavelength/color range (380–780 nm)
- v = measured volts dc

Valid Column Descriptions are listed in the subsections below.

#### 8.3.1 Fluorescence Measurements

CHL=x           sc       off  
 IENGR=x  
 PHYCOCYANIN=x sc       off  
 PHYCOERYTHRIN=x       sc       off  
 URANINE=x sc       off  
 RHODAMINE=x       sc       off  
 CDOM=x       sc       off

#### 8.3.2 Miscellaneous

Date=x           MM/DD/YY  
 Time=x           HH:MM:SS  
 REF=x           Reference Counts—Currently not used by ECOView  
 N/U=x           The column is Not Used



Single sensor fluorometers have optional parameters that can be used to modify either the analog output or the internally calculated engineering units output. To vary the output range of a single sensor fluorometer, use the following parameters:

```
maxvoltage=v  
ASV1=sc1  
ASV2=sc2  
ASV4=sc4
```

where *v* is the maximum output of the sensor, and *scx* is a engineering units per volt scale for each scale setting. Multiply *v* by *scx* to get the maximum output value for each Analog Scale Setting. These parameters will appear on the FL-Setup tab of ECOView.

The internally calculated fluorescence values, the engineering scale, offset, and output can be set by the user from the FL-Setup tab. They are listed below as a reference to the factory settings for the user when the user manually adjusts the scale and offsets that are used in the engineering unit calculations. Engineering units are displayed through ECOView where appropriate. The parameters for changing the internally calculated engineering units are:

```
iengrscale=sc  
iengroffset=off  
iengrunits=label      where label is any continuous character string.
```

## 8.4 Sample Device Files

Below is the standard device file for an *ECO* FLxx, the one used with ECOView host software

```
ECO FL-001 Device File  
Created on: 01/23/03  
  
iengrunits=µg/l  
iengrscaleoffset=4  
  
: LSS=NTU  
: iengrunits = µg/l for CHL, PC, PE. ppb for CDOM and uranine.  
: column 4 = input scale factor and offset.  
  
maxvoltage=4.98  
asv1=6.5  
asv2=12.4  
asv4=26.5  
  
COLUMNS=5  
DATE=1  
TIME=2  
REF=3  
N/U=4  
chl=4    0.0089 85.0  
N/U=5
```



Below is the device file that enables the meter to output processed data (for example, chlorophyll-a) in  $\mu\text{g/l}$ .

```
ECO FL-001
Created on: 01/23/03

iengrunits= $\mu\text{g/l}$ 
iengrscaleoffset=5

: LSS=NTU
: iengrunits =  $\mu\text{g/l}$  for CHL, PC, PE. ppb for CDOM and uranine.
: column 5 = input scale factor and offset.

maxvoltage=4.98
asv1=6.5
asv2=12.4
asv4=26.5

: Has internal CHL in meter output


COLUMNS=6
DATE=1
TIME=2
IENGR=3
REF=4
chl=5 0.0085      6.0
N/U=6
```

## 8.5 Sample Output File

Below is a sample output file for an FLxx. From left to right, columns describe:

Date (MM/DD/YY)	Time (HH:MM:SS)	Reference	Signal	Thermistor
6/1/03	10:03:00	5754	57	531
6/1/03	10:03:01	5740	65	531
6/1/03	10:03:02	5733	67	532
6/1/03	10:03:03	5729	65	531
6/1/03	10:03:04	5725	63	531
6/1/03	10:03:05	5723	62	531
6/1/03	10:03:06	5721	61	531
6/1/03	10:03:07	5719	64	531

## Appendix A: Mounting Bracket Drawing

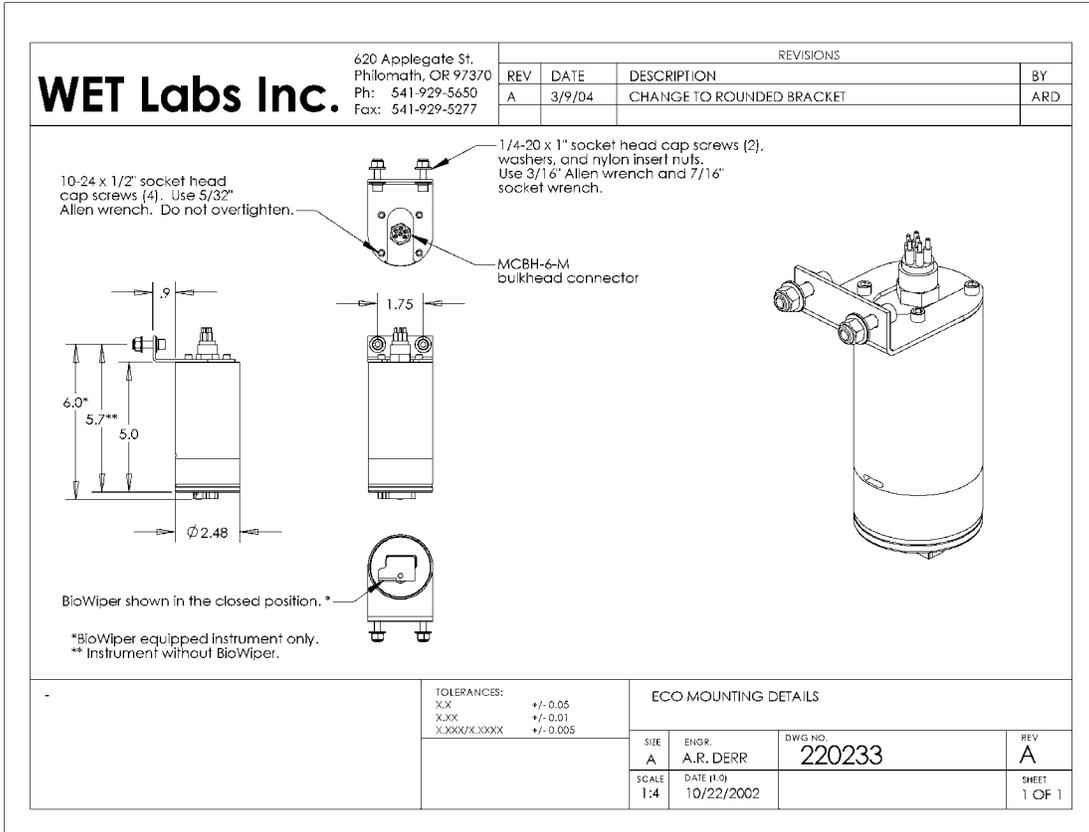

### Revision History

<b>Revision</b>	<b>Date</b>	<b>Revision Description</b>	<b>Originator</b>
A	10/16/02	New document (DCR 242)	W. Strubhar, D. Whiteman
B	10/23/02	Add mounting bracket description (DCR 251)	A. Derr
C	11/12/02	Add analog capability for (RT) models (DCR 254)	I. Walsh
D	2/10/03	Delete battery warning (DCR 272)	D. Whiteman
E	2/24/03	Change "shutter" to "bio-wiper™" (DCR 280)	H. Van Zee
F	3/03/03	Add Terminal Communications section (DCR 283)	I. Walsh
G	4/14/03	Add stop command to terminal communications (DCR 292)	W. Strubhar
H	5/29/03	Add analog signal option to section 3.1.1 (DCR 302)	I. Walsh
I	8/6/03	Add CDOM, Uranine, PC and PE; add deliverable items (DCR 320)	H. Van Zee
J	9/22/03	Correct paragraph in 8.3.2 (DCR 336)	H. Van Zee
K	10/27/03	Correct device file and date format (DCR 341)	D. Romanko
L	11/24/03	Modify explanation for stop data collection command (DCR 342)	W. Strubhar
M	11/25/03	Update specifications table (DCR 338)	I. Walsh
N	2/17/04	Update bio-wiper maintenance and column description for device files (DCR 367)	A. Derr, I. Walsh
O	3/10/04	Add new test cable description, operational description, mounting diagram (DCR 381)	A. Derr, D. Whiteman
P	5/11/04	Update optical specs, remove pin 6 from warning in section 1 (DCR 390)	I. Walsh